# FORA® Test N' GO Advance Voice

## Uric Acid Test System

## *Sistema de medición de ácido úrico*

## Quick Start User Guide / *Guía de Referencia*

For self-testing. Read instructions before use. For *In vitro* diagnostic use. For single patient use only.
**For over the counter use only.**
*Para autoanálisis. Lea las instrucciones antes de utilizarse. Para uso diagnóstico in vitro. Para uso de una sola persona.* ***Solo para uso sin receta.***

Distributed by ForaCare, Inc. / *Distribuido por ForaCare, Inc.*
893 Patriot Drive Suite D, Moorpark, CA 93021 USA
Products made in Taiwan / *Productos hechos en Taiwán*
Toll Free / *Número de Teléfono Gratuito* : 1-888-307-8188 (6:30 am-5:30 pm PST, Monday to Friday / *6:30 am-5:30 pm PST, Lunes a Viernes*)
For assistance outside of these hours, please contact your healthcare professional. / *Para obtener asistencia fuera de estos horarios, póngase en contacto con un profesional de la salud.*
www.foracare.com

315-4183600-010

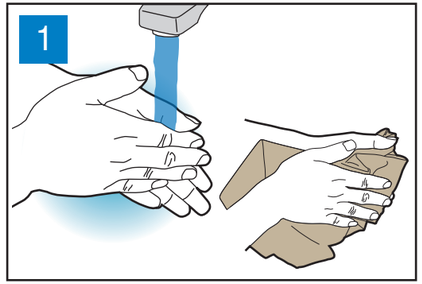


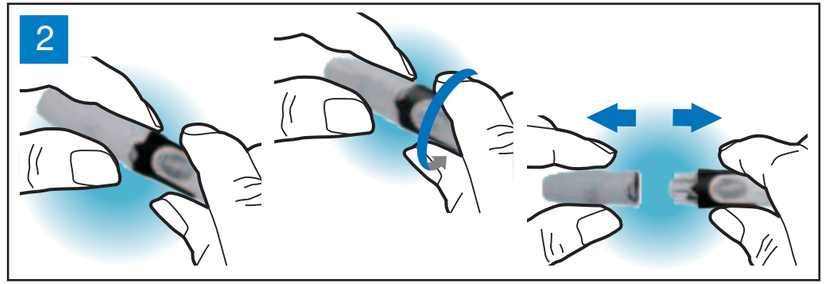


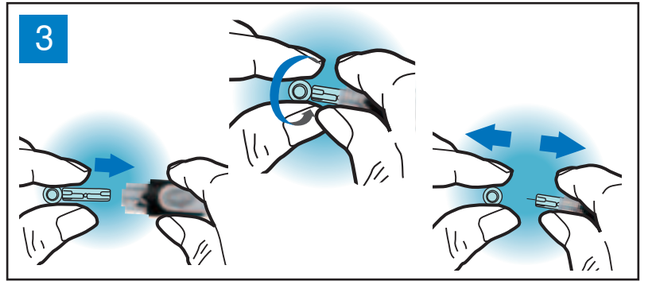


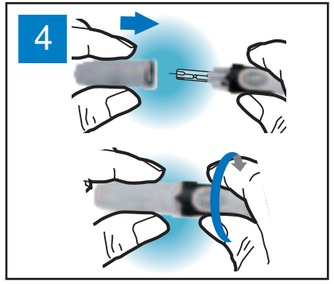








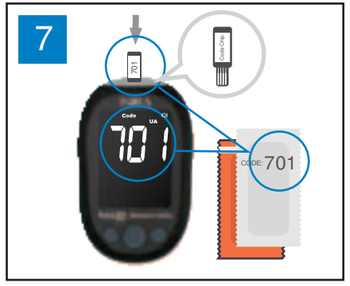


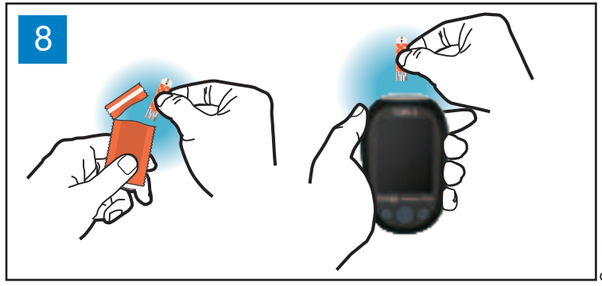


PLACE STAMP HERE
*COLOQUE ESTAMPILLA AQUÍ*

**ForaCare, Inc.**
893 Patriot Drive Suite D
Moorpark, CA 93021 USA

**FORA®** **Five Years Warranty Registration Card /**
***Tarjeta de Registro de Garantía por 5 años***

To save a stamp and receive potential online promotions, please visit https://foracare.com/support/ to complete your product registration.

Name / *Nombre*

E-mail / *Correo Electrónico*

Street Address / *Dirección*

APT#

City / *Ciudad*

Country / *País*

State / *Estado*

Zip / *Código Postal*

Home Telephone / *Teléfono Casero*

Meter Serial Number (See label on back of meter) /
*Número de Serie del Medidor (Ver etiqueta al reverso del medidor)*

Date of Purchase (Month-Day-Year) /
*Fecha de Compra (Mes-Día-Año)*

☐ I acknowledge that ForaCare has the right to contact me with updates, promotions, or meter upgrade offers / *Reconozco que ForaCare tiene el derecho de contactarme con actualizaciones, promociones u ofertas de mejores medidores*

**ForaCare, Inc.** Online Warranty Registration and Detailed Warranty Coverage at www.foracare.com/support.html

9

10



Alcohol pads are not included in the test kit and should be purchased separately.

*Las almohadillas con alcohol no están incluidas en el kit de prueba y deben comprarse por separado.*

11

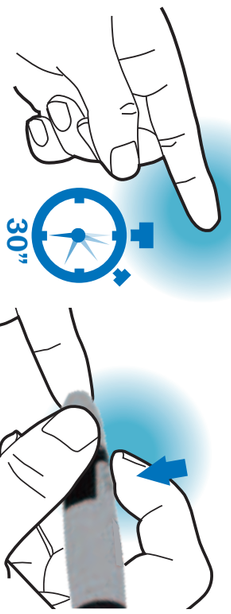


Allow the site to air dry. (If alcohol pad is used.)
Permita que el sitio de prueba se seque al aire. Especialmente si se usa una gasa de alcohol.

12



13

14

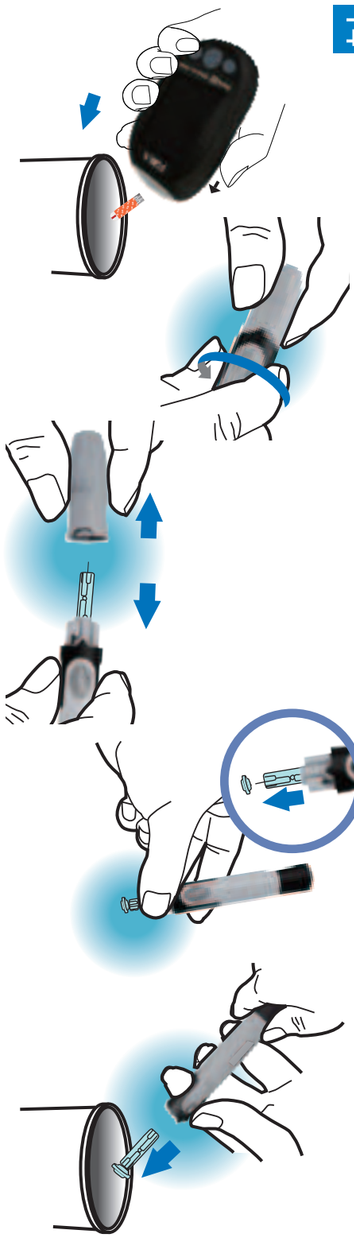

This device is NOT intended for use in healthcare or assisted-use settings such as hospitals, physician offices, or long-term care facilities. Use of this device on multiple patients may lead to transmission of Human Immunodeficiency Virus (HIV), Hepatitis C Virus (HCV), Hepatitis B Virus (HBV), or other bloodborne pathogens.